

# **How Neutrons Are Produced: The NIST Research Reactor and Cold Neutron Source**

**Dr. Robert E. Williams  
Nuclear Engineer  
NIST Center for Neutron Research**



**June 22, 2009**

# Outline

- Nuclear Engineering 101
- Description of the NBSR
- Production of Cold Neutrons
- Evolution of the Liquid Hydrogen CNS
- The Role of MCNP in CNS Development
- Expansion, PeeWee, Liquid Deuterium

# Nuclear Fission of $^{235}\text{U}$


- Because neutrons are emitted in fission, a self-sustaining chain reaction is possible.
- A reactor is critical if exactly one neutron from fission induces another fission.
- 200 MeV/fission is deposited in the core ( $3.1 \times 10^{10}$  fis/sec/watt).
- Slow neutrons are much more likely to cause fission.
  - Thermal reactors

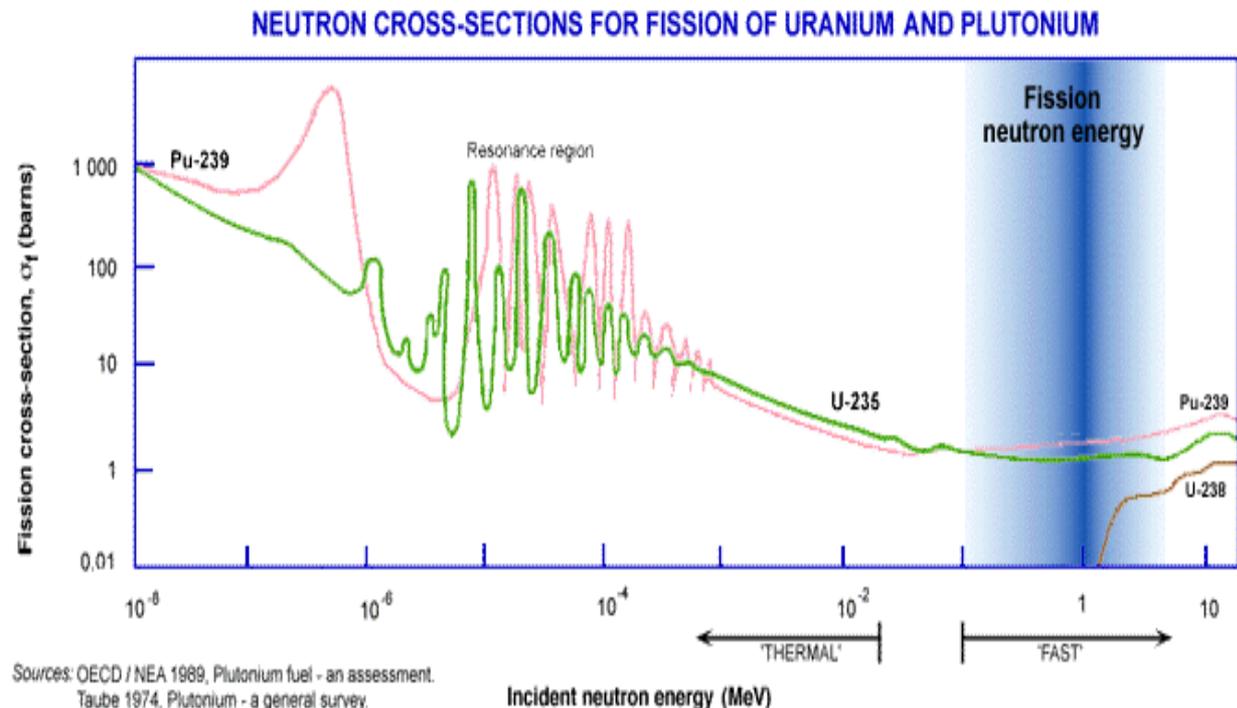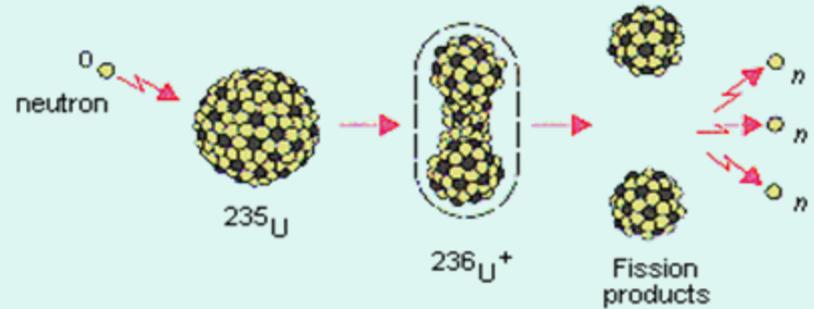

Sources: OECD / NEA 1989, Plutonium fuel - an assessment.  
Taube 1974, Plutonium - a general survey.  
1 barn =  $10^{-28}$  m<sup>2</sup>, 1 MeV =  $1.6 \times 10^{-13}$  J

Incident neutron energy (MeV)

# Thermal Reactor Components

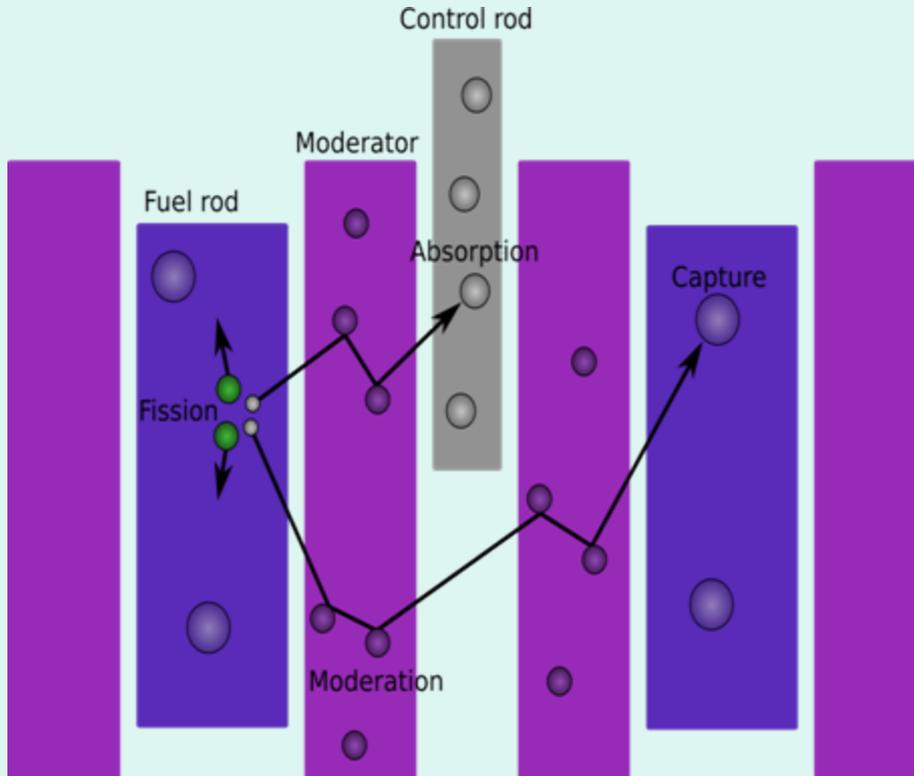

- **Fissile** fuel material, such as  $^{235}\text{U}$ , only 0.7% abundant, or  $^{239}\text{Pu}$ .
- **Moderator** to slow neutrons ( $\text{D}_2\text{O}$ ,  $\text{H}_2\text{O}$ , Graphite)
- Control Elements (Cd, B)
- Reflector, Shielding, Coolant, Neutron source and detectors
- Early Reactors:
  - Oklo, Gabon -1.7 billion B. C. E. (U ore +  $\text{H}_2\text{O}$ )
  - Univ. of Chicago – 1942 (Natural U + graphite)

# Reactor Kinetics and Control

The neutron ***Multiplication Factor***,  $k$ , is

$$\frac{\text{Number of fissions in one generation}}{\text{Number of fissions in the previous generation}}$$

$k = 1.000$  for a critical reactor at steady power. ***Reactivity***, approximately  $k-1$ , measures the departure from critical.

The neutron lifetime in most reactors is about  $100 \mu\text{sec}$ . One generation?

Let  $k = 1.001$ , for example. If the fission rate increased by 1.001 every  $10^{-4}$  sec, the power would increase a factor of  $(1.001)^{10,000} = 22,000$  in one second,  $5 \times 10^8$  in 2 seconds, etc. Oops!


Fortunately, about 0.7% of the neutrons are delayed; they are emitted in the beta decay of fission products, spanning thousands of “generations”.

Slow moving control rods and negative power coefficients keep the reactivity well below 0.007, so the power increase is manageable.

# NIST Research Reactor History

- Designed in the 1960's, and included a beam port for a cold neutron source.
- First Critical, December 7, 1967.
- 10 MW until 1985, 20 MW since.
- D<sub>2</sub>O Cold Neutron Source installed, 1987.
- First neutrons in the guide hall in 1990.
- LH<sub>2</sub> Source installed September 1995
- Advanced LH<sub>2</sub> CNS, Unit 2, installed 2002.

North 

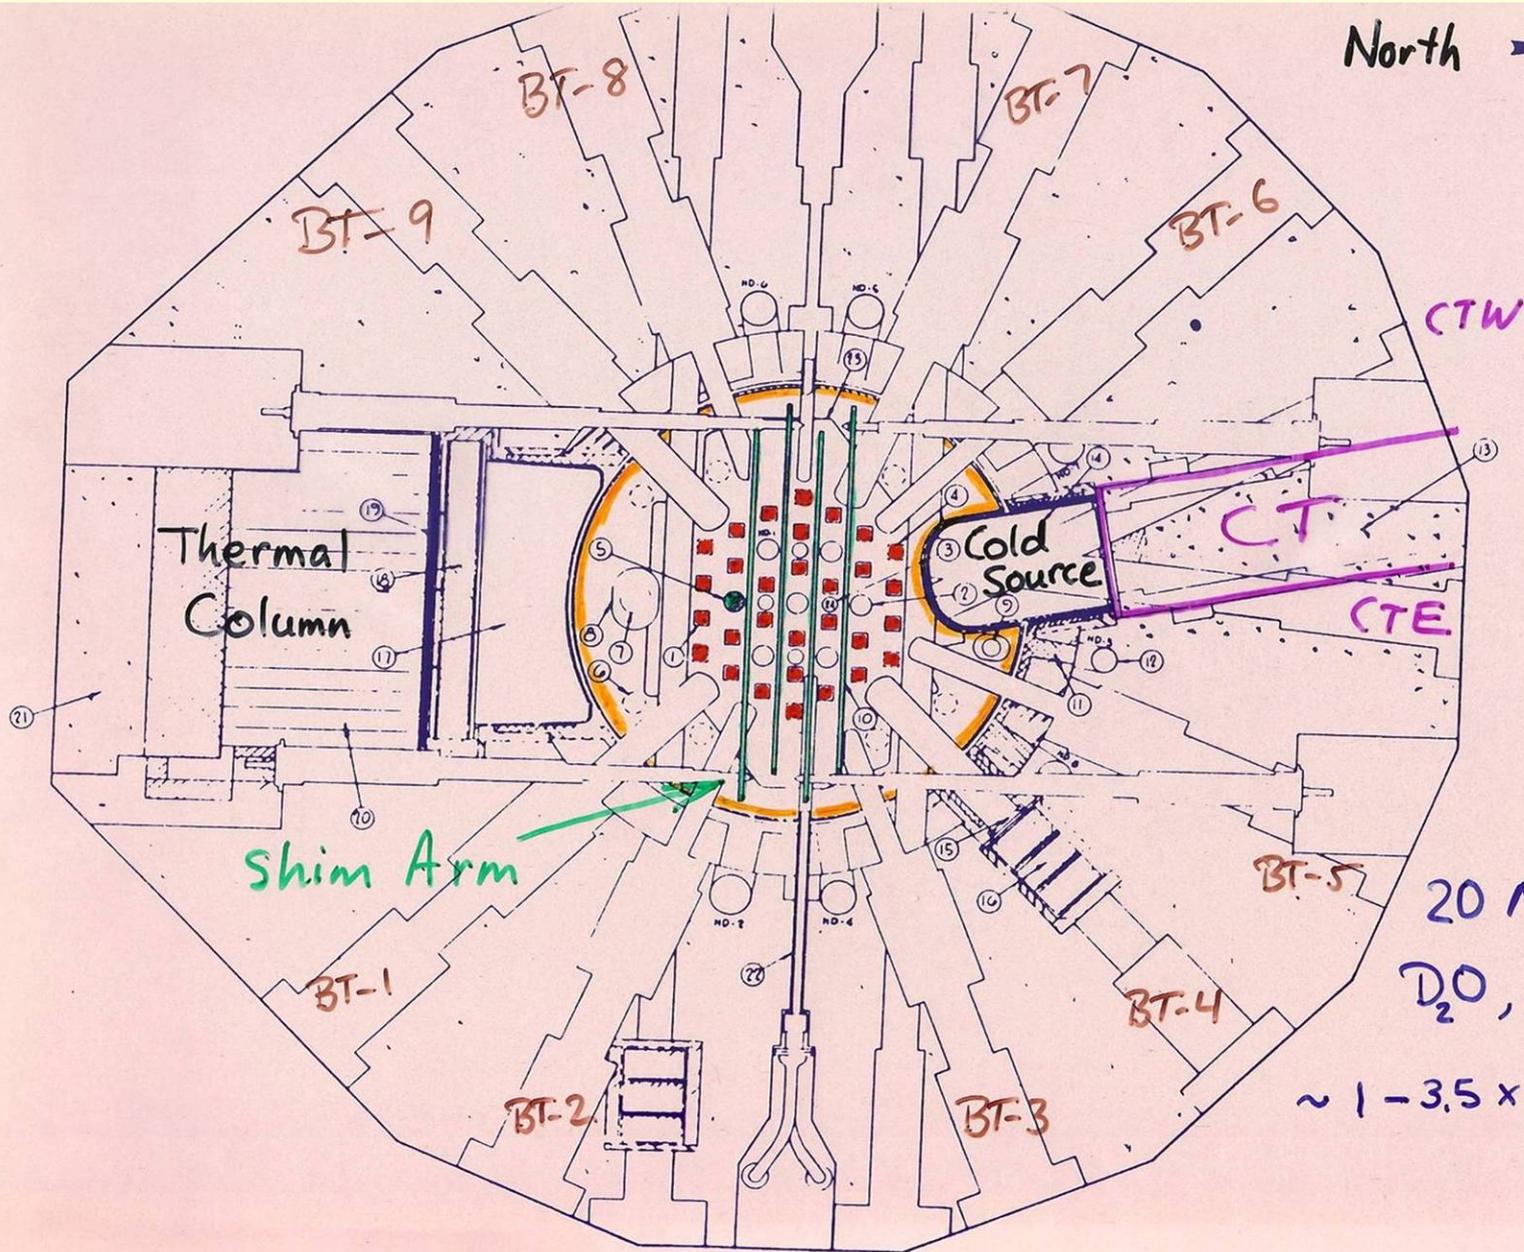

1. FUEL ELEMENT
2. 3/4 EXPERIMENT
3. 1/4 EXPERIMENT
4. SPARE FUEL E
5. REGULATION R
6. LOCATION OF 6
7. IN TOP SHIELD
7. FUEL ELEMEN
8. TOP REFLECTO
9. OVERFLOW PIP
10. SHIM SAFETY
11. LEAD NEUTRO
12. SHIELD FOR IN
13. VERTICAL INST
14. COLD NEUTRON A
15. SUBSTITUTE CO
16. BEAM TUBE CO
17. VERTICAL SHUT
18. THERMAL COOL
19. BISMUTH SHIELD
20. BORAL CURTAIN
21. GRAPHITE
22. THERMAL COLUMN
23. PNEUMATIC TUBE
24. HEAVY WATER
25. TEMPORARY ST.


20 MW

D<sub>2</sub>O, HEU

~ 1 - 3.5 x 10<sup>14</sup> n/cm<sup>2</sup>/s

# Reactor Core Characteristics


- **High Enrichment U Fuel: 93%  $^{235}\text{U}_3\text{O}_8$  + Al**
- **D<sub>2</sub>O Coolant, Moderator, Reflector**
- **30 fuel elements**
  - Fuel cycle 38 days
  - Load 4 fresh elements, reposition the others
- **Peak Flux:  $3.5 \times 10^{14}$  n/cm<sup>2</sup>/sec**
- **9 radial thermal neutron beams**
  - mid-plane (un-fueled region)
  - $1.5 \times 10^{14}$  n/cm<sup>2</sup>/s
- **5 “rabbits” and 10 vertical thimbles for sample irradiations**

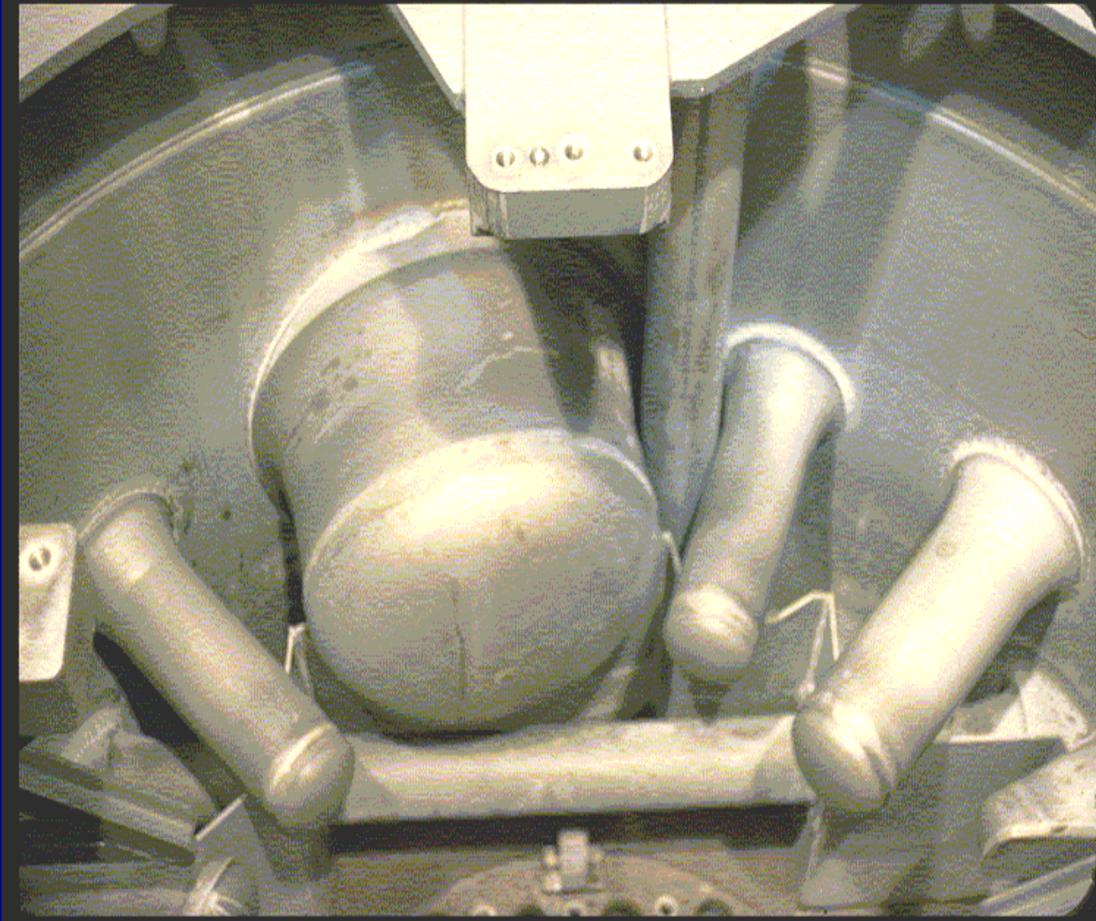

**Interior of the NBSR vessel, showing BT-6, CT, BT-5 and BT-4 thimbles. The Cryogenic Thimble is 55 cm ID.**

# Cut-away View of the NBSR Core

- Looking inside Al reactor vessel
- 18-cm gap (5) between the upper and lower fuel (18)
- Semaphore-type Cd shim arms (2)
- D<sub>2</sub>O flow inside the fuel elements
- CNS (15) visible in cutout CT thimble

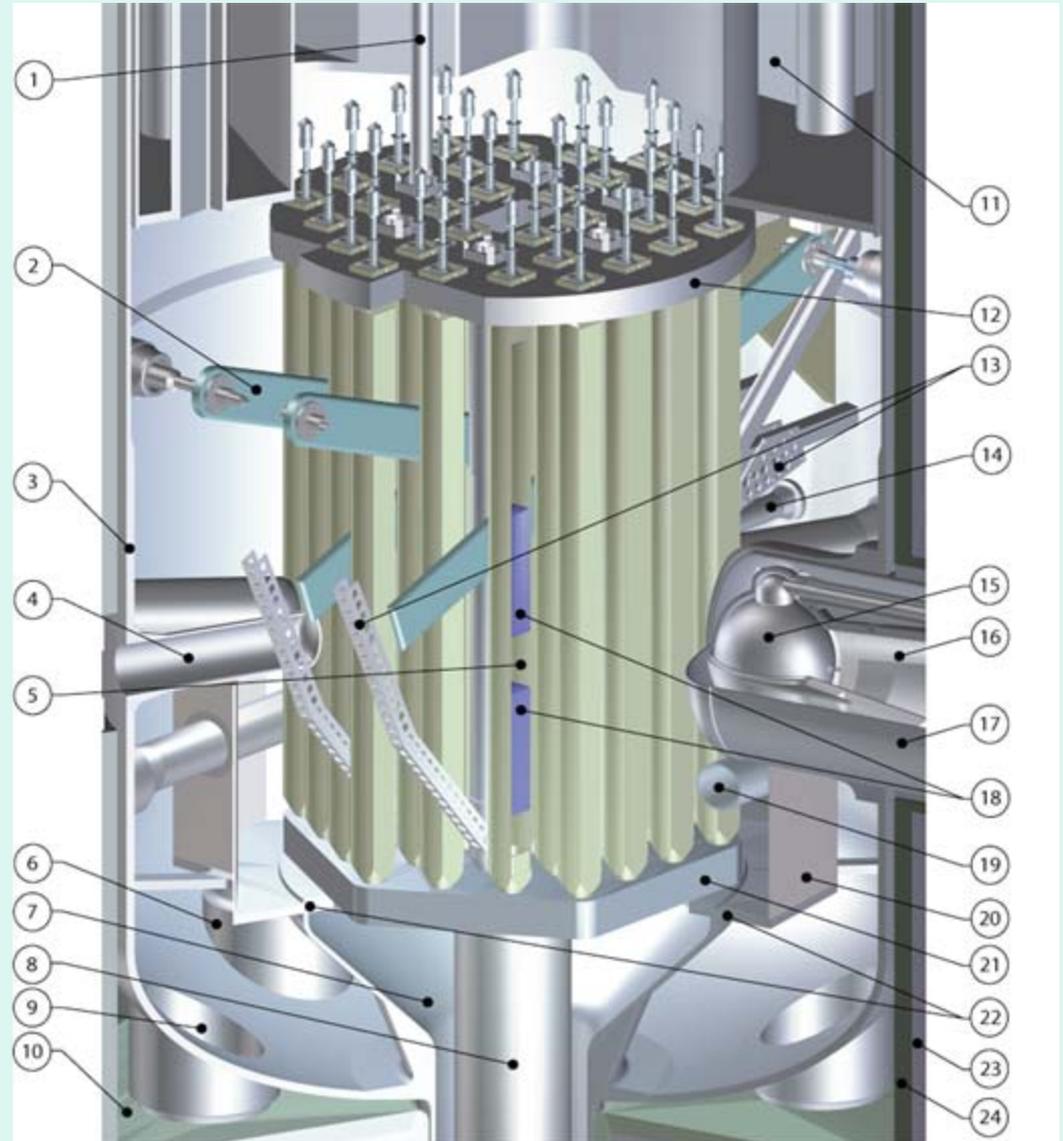


# Production of Cold Neutrons

- The neutrons born in fission have an average kinetic energy of about 2 *Mega*-electron volts, 2 MeV.
- They are slowed to thermal energies (20 – 400 *milli*-eV) by scattering from the molecules of the heavy water (D<sub>2</sub>O) moderator in the reactor. The D<sub>2</sub>O is about 108 °F, or 315 Kelvin.
- In thermal equilibrium, the neutron energy spectrum is determined solely by the temperature of the moderator (a Maxwell-Boltzmann distribution), analogous to the motion of atoms in an ideal gas.

To reach lower energies, therefore, we introduce a cold moderator, such as liquid hydrogen at 20 K.

# Effect of an Ideal Cold Moderator on the Neutron Flux Energy Spectrum

- The Maxwell-Boltzmann energy spectrum is
- $\Phi_{th}(E) = [C / T^{3/2}] E \exp(-E/kT)$
- In the limit of  $E \rightarrow 0$ , the maximum theoretical gain of a cold source at 20 K with respect to a thermal spectrum at  $T_0 = 315$  K is:
  - The LH<sub>2</sub> source had a maximum gain of about 45.
  - “Effective” temperature is 38 K

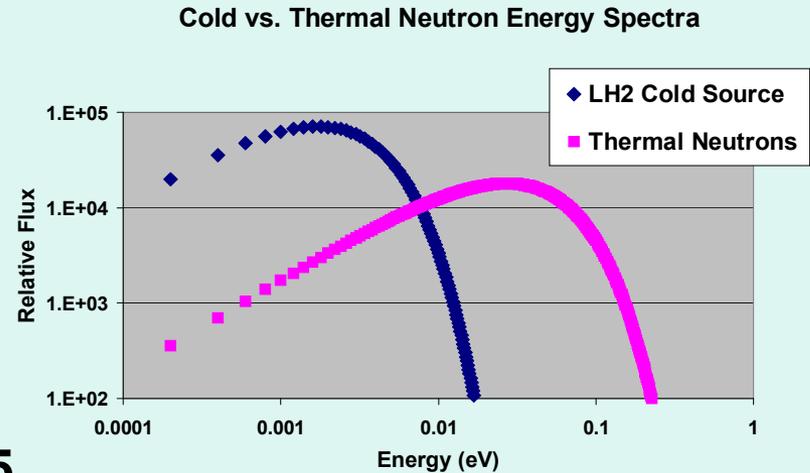

Moderator Temperature (K)	Most Probable Energy (meV)	Wavelength (Angstroms)
315	30	1.6
20	2	6.4

# Original Plan View of NBSR

For the first 20 years, there was **NO** cold source!

CT thimble filled by a  $D_2O$  tank, with BT's along CTE and CTW.

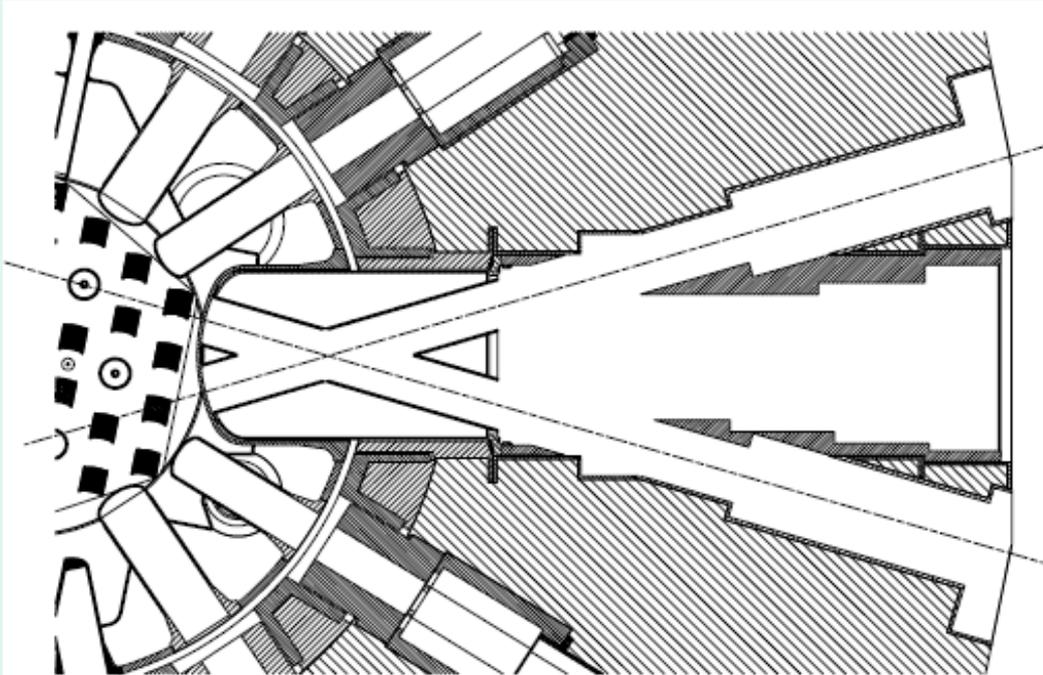


Figure 2.2. Original layout of the cold neutron port.

CTW


CTE and CTW are NOT radial beam tubes.

They intersect at the point of the planned CNS.

CTE


# NBSR Designed for a D<sub>2</sub>O Ice Source

- Cryostat made of Mg
- 16 liters of ice at 30-35 K
- A Lead/bismuth shield (water cooled) required to reduce nuclear heating
- Optimum source contained 8% H<sub>2</sub>O (ice)
- Operated from 1987 to 1994
- Operational difficulties, but gain of 3x in cold neutrons
  - Unpredictable stored energy releases from recombination

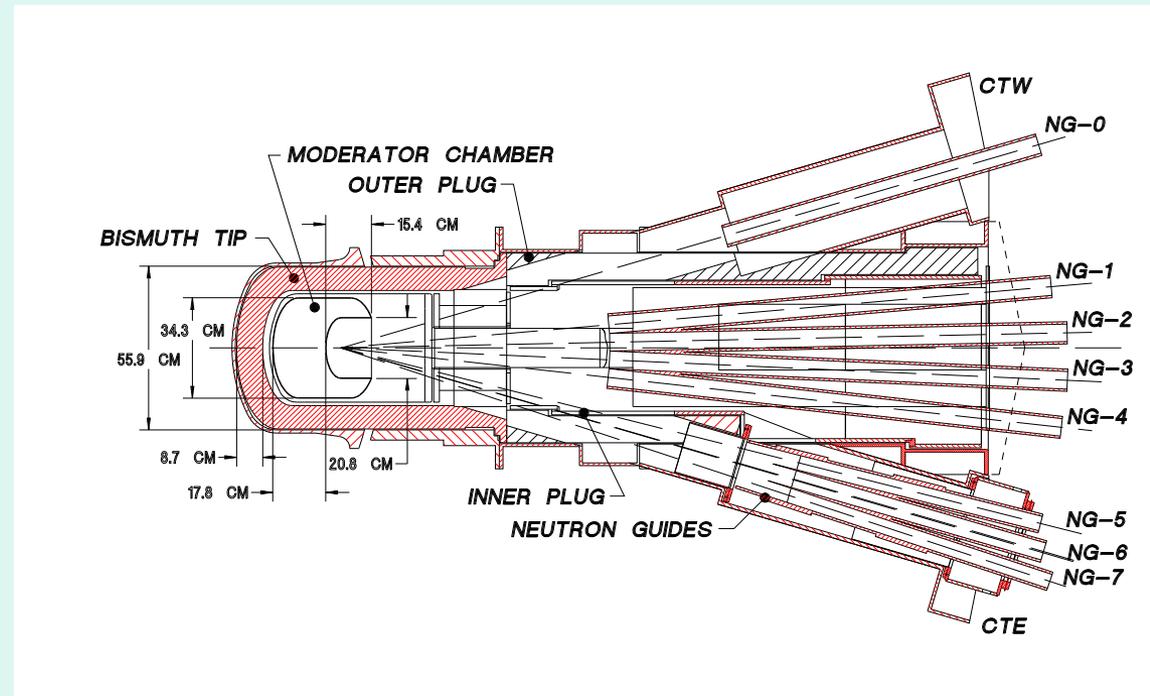

***Every 2 days, we had to "burp" the cold source!***

# The LH<sub>2</sub> CNS, Unit 1, installed in 1995, had a gain of 6 times the D<sub>2</sub>O source

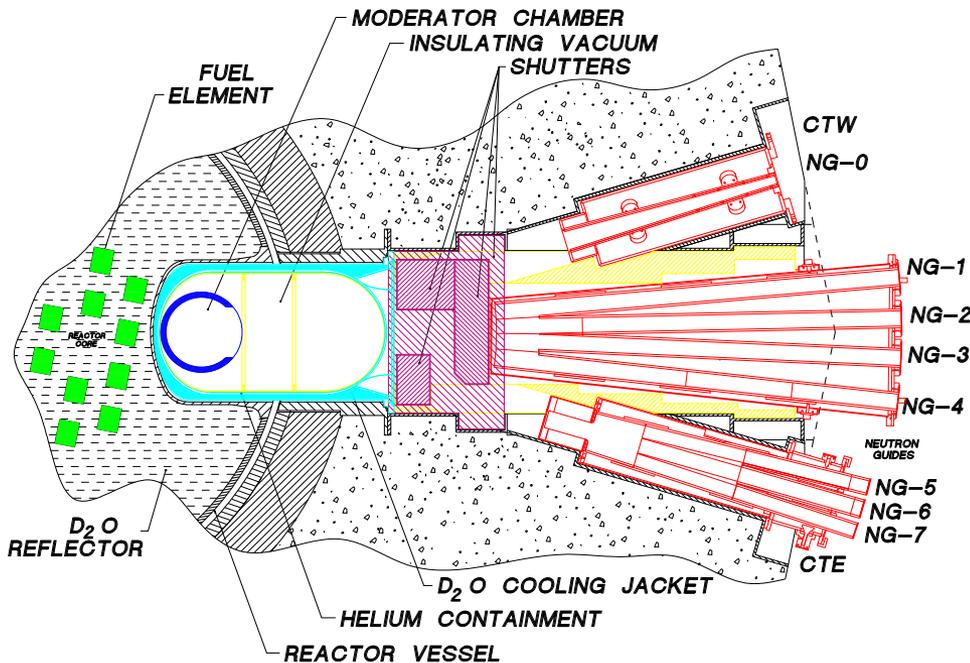


To fully illuminate the beam ports, the source had to have a very large area.

A 320-mm spherical annulus, 20 mm thick, with a 200-mm diameter exit hole was chosen:

- Low heat load (850 W)
- Ease of fabrication.  
Material: Al 6061-T6
- Composed of concentric Al spheres (5 liters of LH<sub>2</sub>)
- Hydrogen vapor filled the inner sphere, which was open at the bottom.

# The Advanced Liquid Hydrogen Cold Source – March, 2002

- Our computational (MCNP) model of the reactor core evolved since the initial design of the LH<sub>2</sub> cold source.
- Simulations showed that expanding the volume of D<sub>2</sub>O around the moderator chamber would better couple the source to the core.
- Several changes were incorporated in Unit 2:
  - Expanded the D<sub>2</sub>O cooling jacket to partially surround the moderator.
  - Eliminated the vapor-filled region in the interior.
  - Used a smaller chamber and a thicker annulus for LH<sub>2</sub>.
- The hydrogen condenser, ballast tank, refrigerator and I&C systems were unchanged.

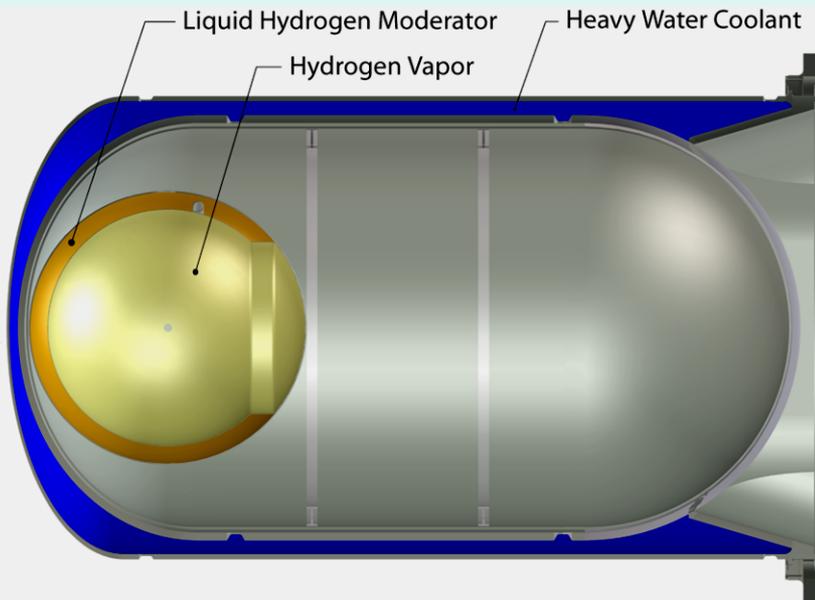

***Hydrogen Cryostat Unit 1***


Unit 1 had too much empty space next to the reactor core.

Vapor in the inner sphere scattered cold neutrons from the beam.

Much more  $D_2O$  in Unit 2 results in a higher neutron flux in the CNS region and the adjacent fuel elements.


32 x 24 cm ellipsoid allows more  $D_2O$  and a thicker  $LH_2$  annulus.

Vacuum filled inner ellipsoid.

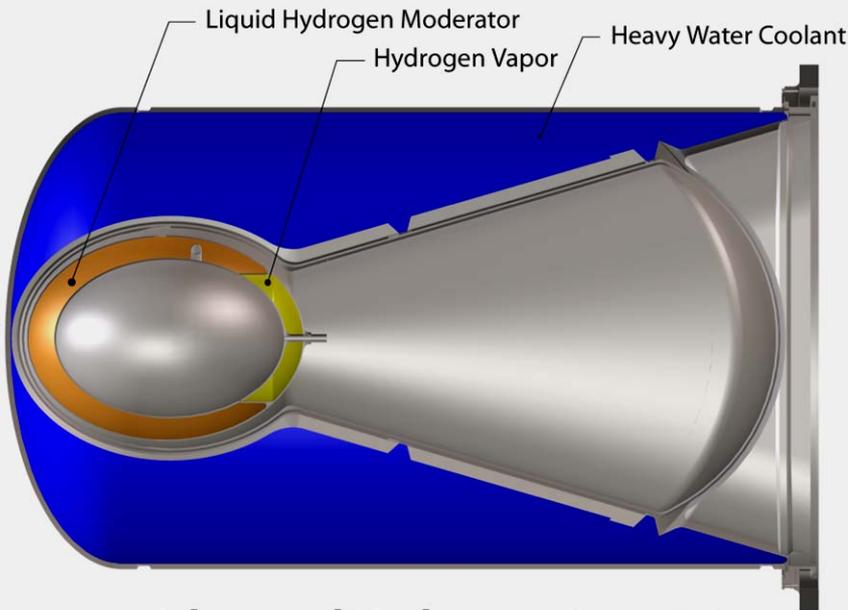


***Advanced Hydrogen Cryostat***

**The condenser is located outside the reactor, 2 meters above the source**

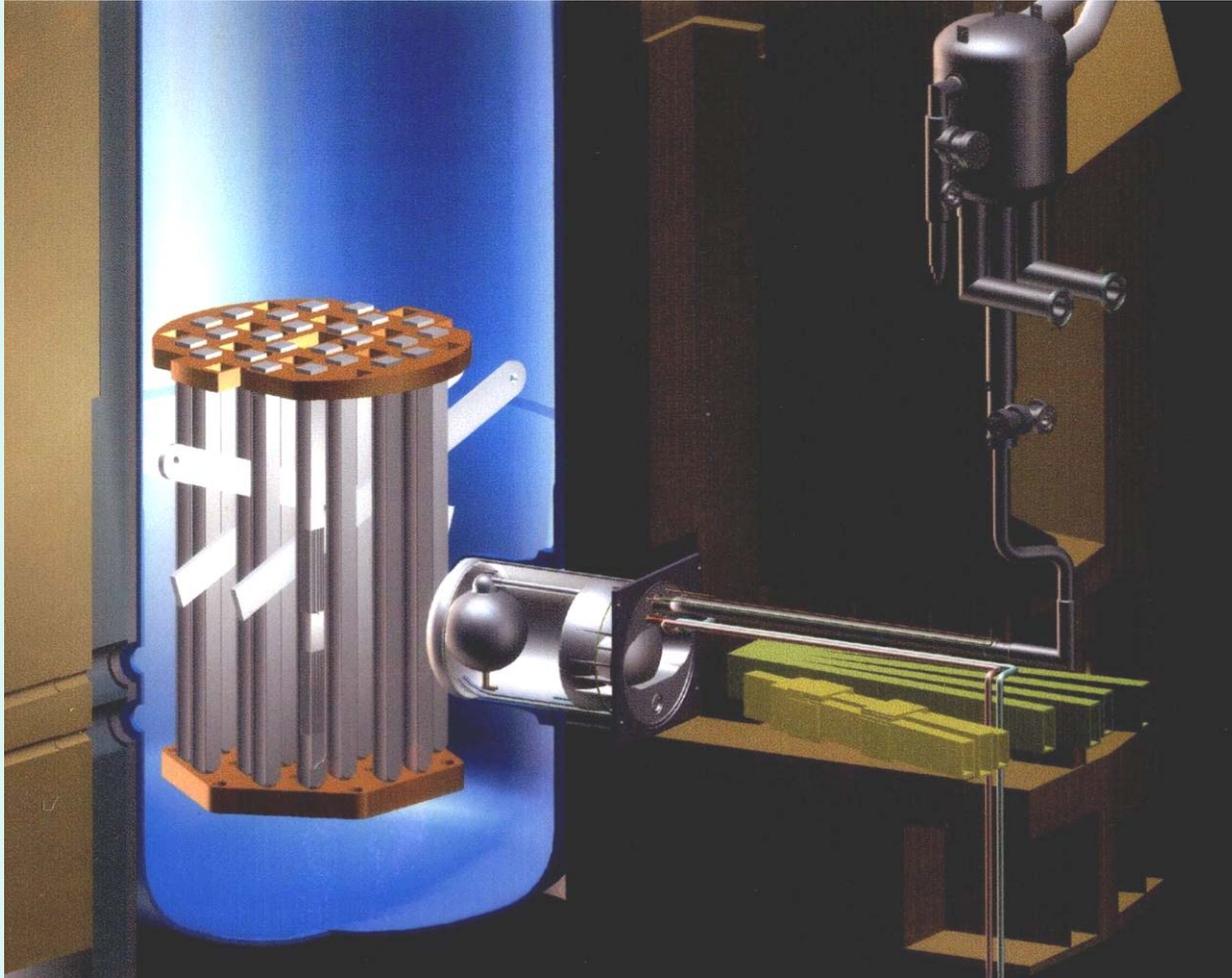

# The liquid hydrogen cold source is passively safe, simple, and reliable

- A thermosiphon is the simplest way to supply the source with LH<sub>2</sub>.
  - Cold helium gas cools the condenser below 20 K.
  - Hydrogen liquefies and flows by gravity to the moderator chamber.
  - Vapor rises to the condenser and a naturally circulating system is established.
- Thermal hydraulic tests showed a thermosiphon could safely remove at least 2200 watts.
- ***The system is closed to minimize hydrogen gas handling.***
- All system components are surrounded by He containments.


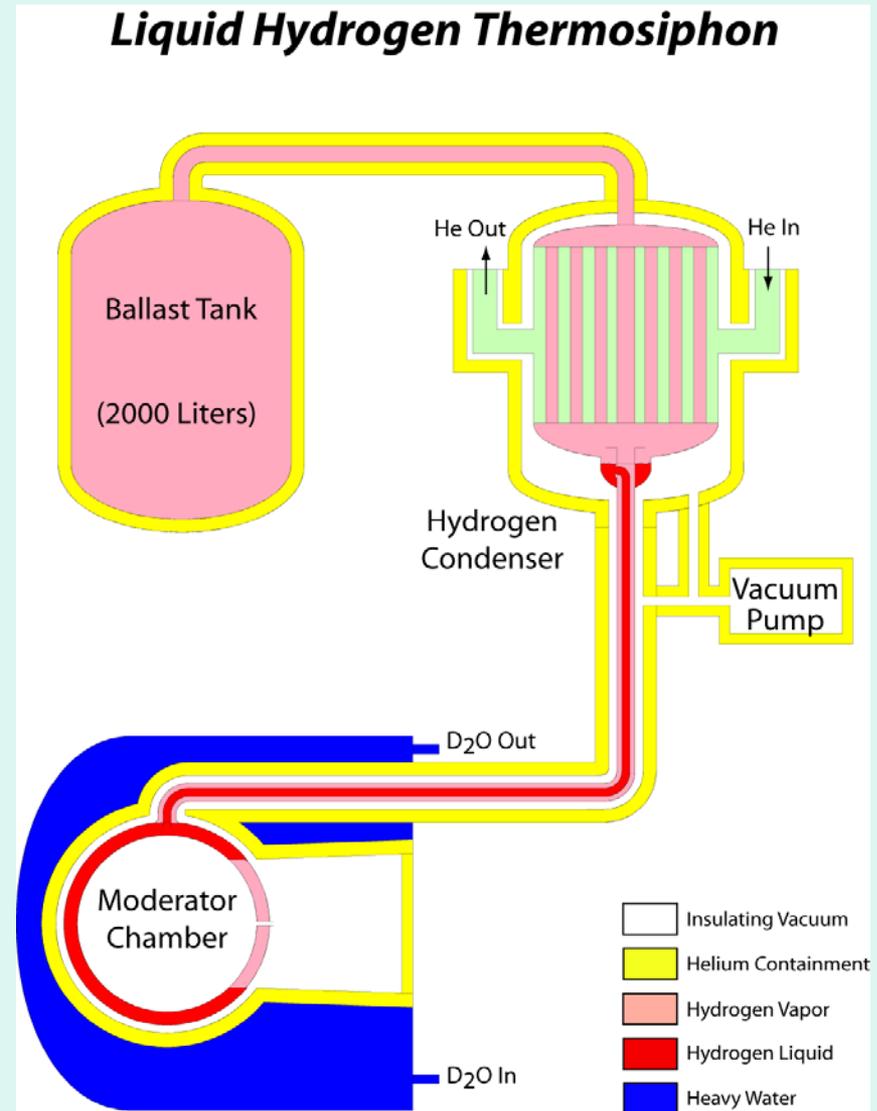


# The MCNP Model of the NBSR

- MCNP (Monte Carlo Neutron-Photon) is a transport code with generalized geometry:
  - Cold moderator cross section data
  - Criticality calculations for reactor normalization
- Initially used to model the cold source region for performance and heat load calculations.
- 30 fuel elements in a hexagonal array, with all 1020 fuel plates, cladding, coolant, etc.
  - 30 fuel materials with varying burn-up
  - Each step for the 7- and 8- cycle fuel elements
  - Shim arms, regulating rod, beam tubes, etc.
- MCNP was used extensively in the updated SAR for the reactor relicensing effort.

The MCNP model of the NBSR was created for CNS development.

The code has generalized geometry and scattering kernels for cold moderators, and powerful variance reduction techniques to tally low-probability events.

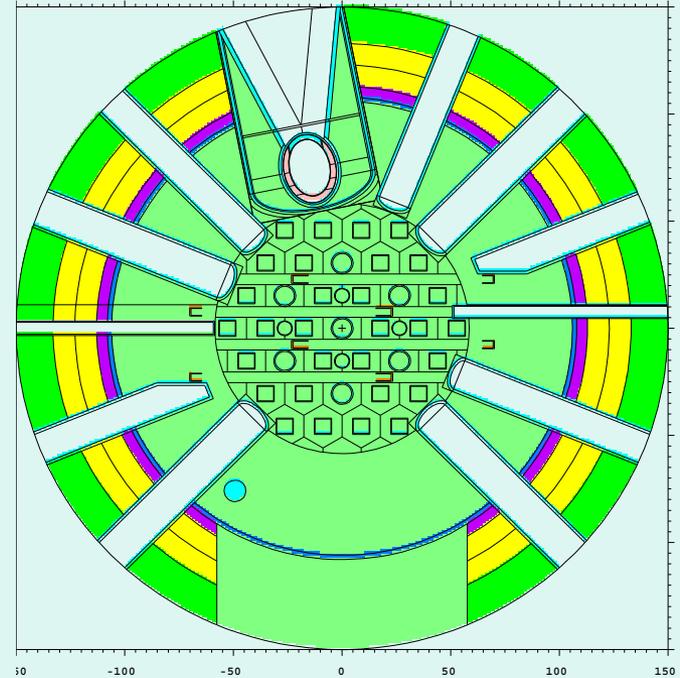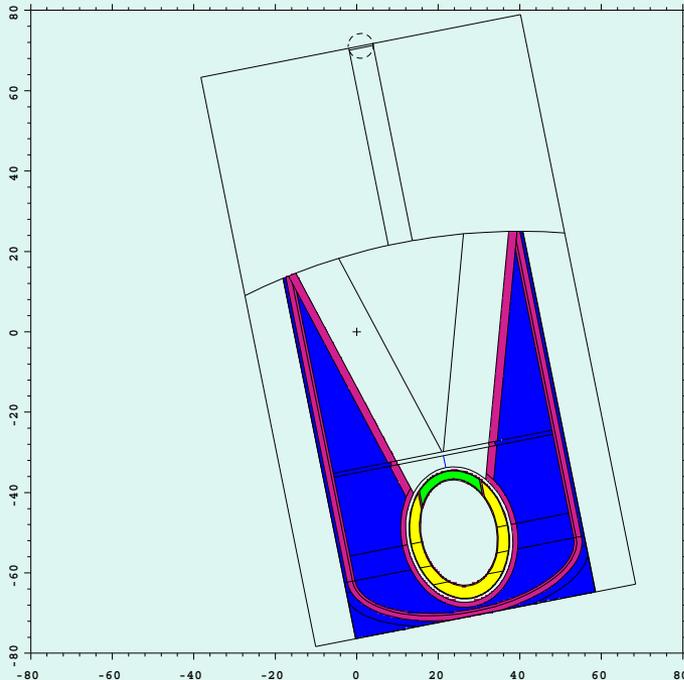


A surface source was generated from the whole-core criticality calculation for CNS performance calculations.

This source preserves the normalization.

The DXTRAN feature was used to force “pseudo” particles to a current tally plane at the neutron guide entrance.

# A second LH<sub>2</sub> source is being developed as part of the NCNR Expansion Initiative

- 5 new guides will be installed in CTW for the guide hall expansion.
- MACS will be moved to BT-9 and have its own small LH<sub>2</sub> source.
- “PeeWee” has an 11-cm ID, and a 0.5-l volume.
- It will have a gain of about 1.7 compared to Unit 2.

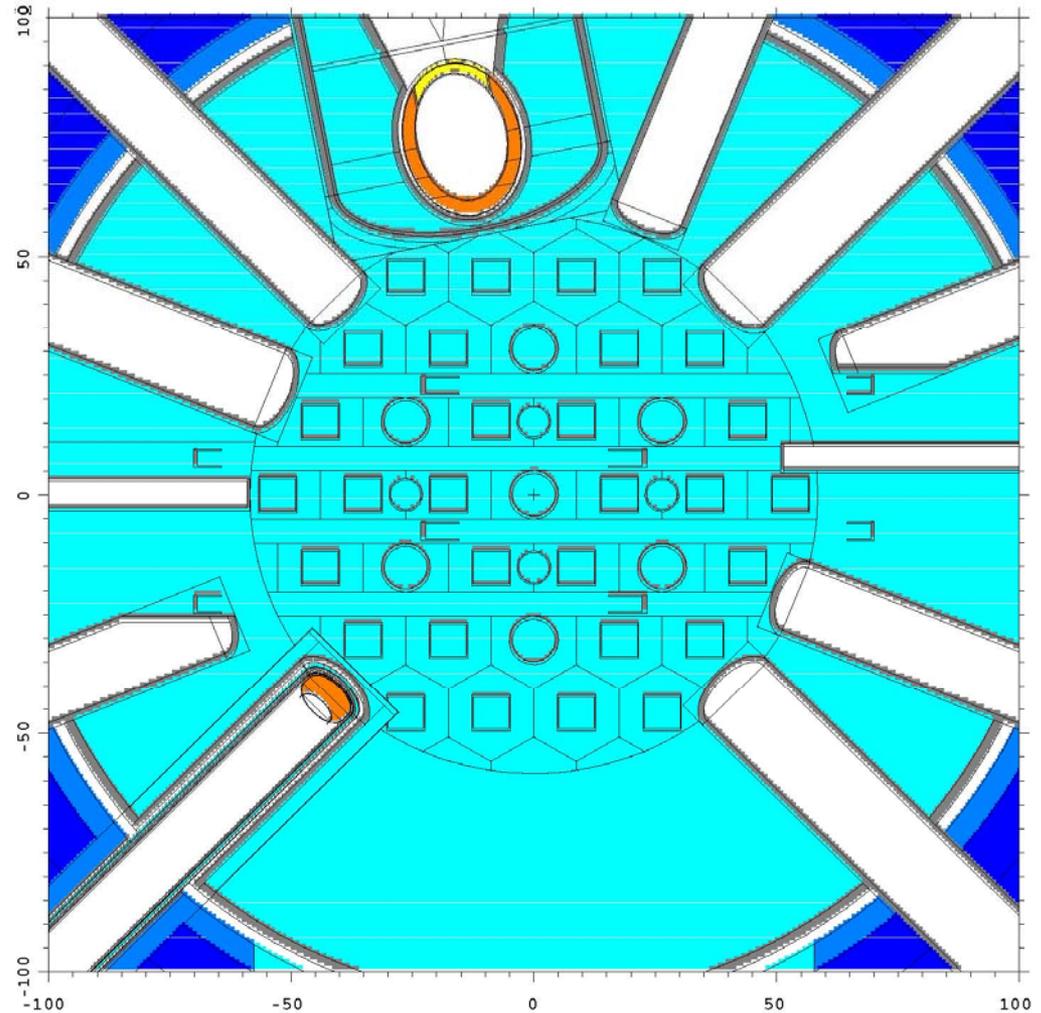

# Unit 3: A Liquid Deuterium Source for NBSR?

A 42 x 42 cm liquid deuterium source in the CT thimble.


Large volume: 45 liters

Deuterium inventory would be many times our H<sub>2</sub> inventory.


10 kg @ 500 kPa will have an expansion volume of nearly 15 m<sup>3</sup> (8 times our ballast tank)

Big investment in metal hydride storage units may be needed to contain tritium.

Calculated heat load of 4 kW will require a new refrigerator, which we are buying with ARRA funds.

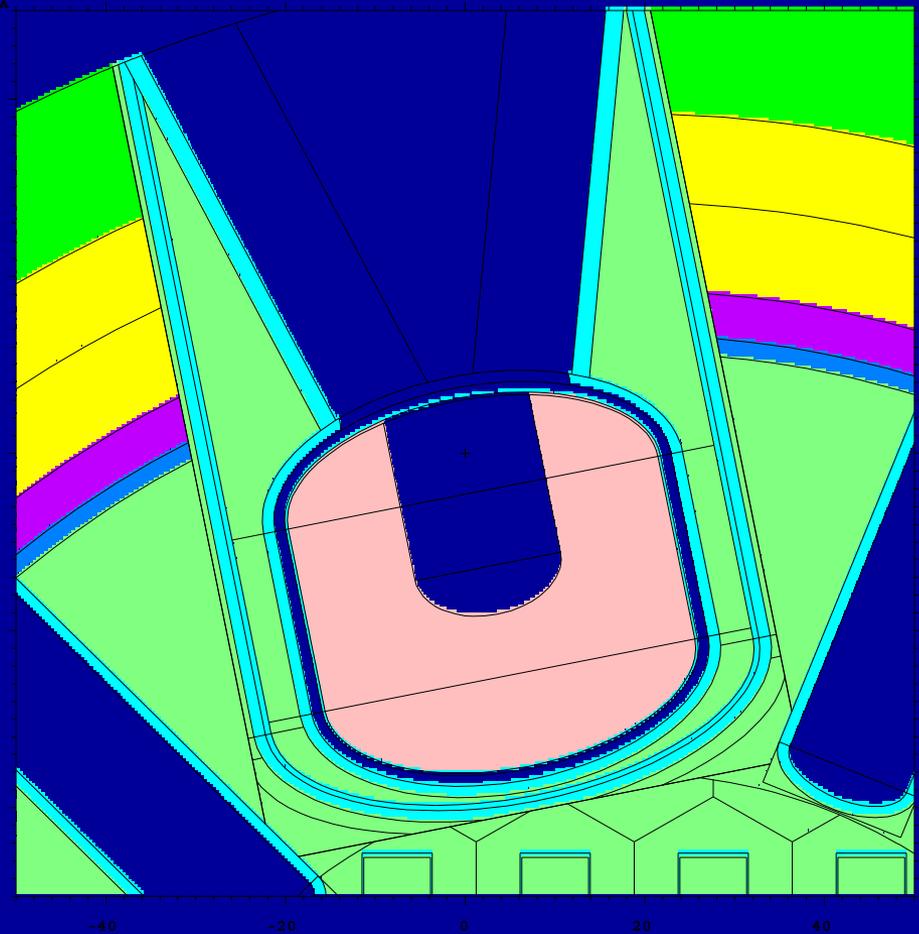

# Relative Brightness of a 45-liter LD<sub>2</sub> CNS vs. Unit 2, 0 – 20 meV

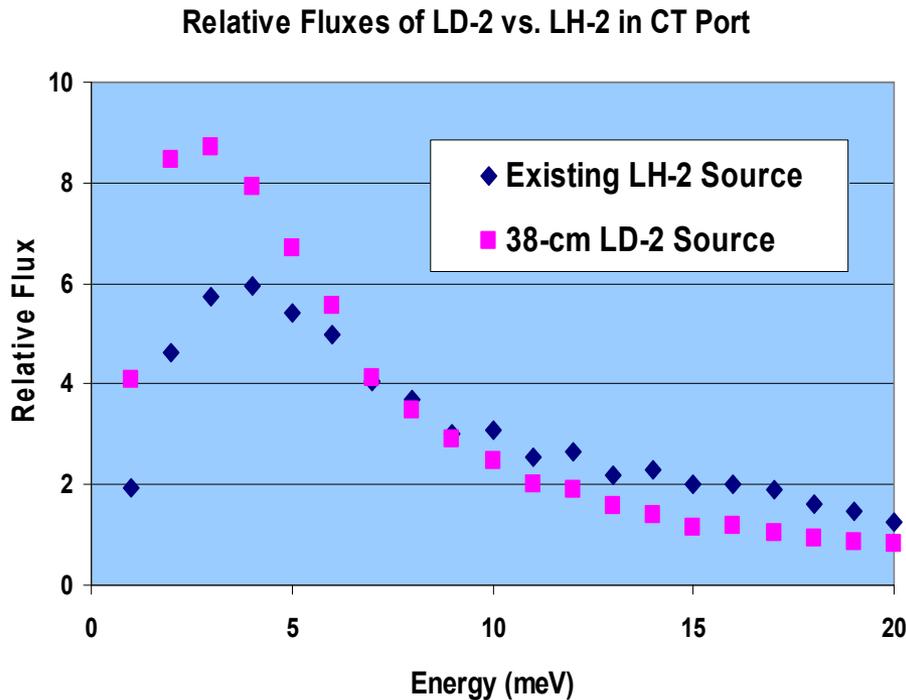

- Spectrum shifts to lower energies.
- Gain greater than 2 for the longest wavelengths.
- Maxwell-Boltzmann temperature drops from 38 K to 28 K.
- Small loss of intensity for 5 - 10 meV.
- Up to 50% loss at 15 meV (2.5 Angstroms).

# Conclusion

- 2007 marked 40 years since the first criticality of the NBSR.
  - 20<sup>th</sup> anniversary of the first cold source
- We continue to explore ways to better utilize the facility.
  - Cold source upgrades
  - Expansion of guide hall with 5 new cold guides
  - Advances in optics, instrument development
- Soon our operating license will be renewed for 20 years by the NRC.